

#### Conditions for delivery and release of surgical face masks

Versie 2020.03.28

Different types of face masks can be used as a means of prevention of and protection against the transmission of the SARS-CoV-2 virus: surgical face masks and respiratory protection masks (so-called "dust masks").

• **surgical or medical masks**: these masks are medical devices and the competent authority is the Federal Agency for Medicines and Health Products (FAMHP).



Surgical masks are designed to protect the patient from contact with infectious agents and particles from the medical staff. But they might also be intended to be worn by patients and other persons to reduce the risk of infections spreading, for example in epidemic or pandemic situations. Surgical face masks are class I medical devices. They need to comply with the requirements of the <u>Royal Decree of 18/03/1999</u> on medical devices (transposition of the <u>European Directive</u> <u>93/42/EEC</u> – 'MDD') or with the requirements of the <u>European Regulation 2017/745</u> on medical devices ('MDR').

The European harmonised standard these masks have to meet, is EN 14683 "Medical face masks – Requirements and test methods".

More information on medical devices can be found on our <u>website</u>.

 respiratory protection masks (Type FFP2/FFP3 dust masks): these products are personal protective equipment (PPE) and the competent authority is the Federal Public Service of Economy, SMEs, Self-employed and Energy. More information on PPE can be found on the website of <u>FPS</u> <u>Economy.</u>





e.g.

#### Conditions for delivery of surgical face masks before release is allowed

The compliance of surgical face masks with the essential requirements as described in the legislation, needs to be assessed by the manufacturer. The manufacturer (or his authorised representative) confirms the compliance of the products in a 'declaration of conformity' ('DoC') that should be available to clients. Compliant products that are not placed on the market in sterile conditions shall bear the CE marking as in the figure below. A CE certificate issued by a notified body ('NB') is not necessary for non-sterile surgical face masks.



Sterile surgical face masks need to bear a CE marking followed by a 4-digit code. See also figure below. These 4 digits identify the notified body that assessed the elements for securing and maintaining the sterile conditions. The notified body issues a CE certificate for this purpose.

# CE

#### e.g.

The CE marking needs to be present on the masks themselves or, when this is not possible, on the packaging/labelling of the masks. It should also appear on the sales packaging (e.g. boxes) and in the instructions for use (if present).

Considering the exceptional situation, we allow for deviations from these rules for CE marking and conformity assessment as described in <u>European Recommendation 2020/403</u> of the European Commission of 13 March 2020 on conformity assessment and market surveillance procedures in the context of the COVID-19 threat.

# Surgical face masks that do not bear the CE marking may be accepted exceptionally and temporarily, provided that it is ensured that the products are made available only during the current crisis and do not enter regular distribution channels.

For the conformity assessment of surgical face masks, the FAMHP will also exceptionally accept test results according to international standards that can be considered equivalent to EN 14683.

These alternatives might be:

#### • USA: ASTM F2100

China: YY 0469:2011 and YY/T: 0969-2013

Conformity can be demonstrated by test reports or by a third party certificate. If sufficiently documented (certificates, test results according to an equivalent standard, accredited laboratory and possibility to link all documents to the batches or goods concerned), this may be accepted as an alternative.

Currently we find that Chinese masks are being tested according to European standards (for example the standards EN 14683, EN 149) by Chinese laboratories/testing bodies. Normally, compliance with European standards can only be confirmed by European testing labs with an accreditation to do so, but if the laboratory or inspection body figures on the following list of bodies that are accredited by

FAMHP

the Chinese Authorities, their certificates will also be accepted (please also see <a href="https://www.cnas.org.cn/english/findanaccreditedbody/04/896740.shtml">https://www.cnas.org.cn/english/findanaccreditedbody/04/896740.shtml</a>).

Testing reports from laboratories that are **not on this list, will not be accepted**.

#### Which documents should definitely be present?

- **For non-sterile surgical face masks with CE marking:** EU declaration of conformity from manufacturer (or authorised representative)

#### - For sterile surgical face with CE marking:

EU declaration of conformity from manufacturer (or authorised representative) CE certificate for the sterile aspects, issued by a notified body that is designated for medical devices under <u>Directive 93/42/EC</u> (MDD)or under <u>Regulation 2017/745</u> (MDR)

- **For surgical face masks without CE-marking:** Testing reports from accredited lab/certificate from a third party Identification of the alternative standard that was used

### Offers that are not accompanied by the aforementioned documents will NOT BE TREATED. Deliveries that are not accompanied by these documents will NOT BE RELEASED.

All documents should be linkable to the products in an unambiguous way. Pictures of the product, its packaging and labelling can be added as support in the offer.


Conditions for delivery of respiratory protection masks (FFP2/FFP3) release is allowed

For these masks, all conditions can be found on the website of the FPS Economy using the following <u>link</u>.

## ATTENTION: falsified certificates

We bring to your attention that falsified and irrelevant certificates are circulating for surgical face masks and FFP masks, pretending to prove their conformity to European rules.


Below, some examples are presented that were recently seen by the Belgian Authorities. More information and more examples can also be found on the <u>website of the European Safety Federation</u>.

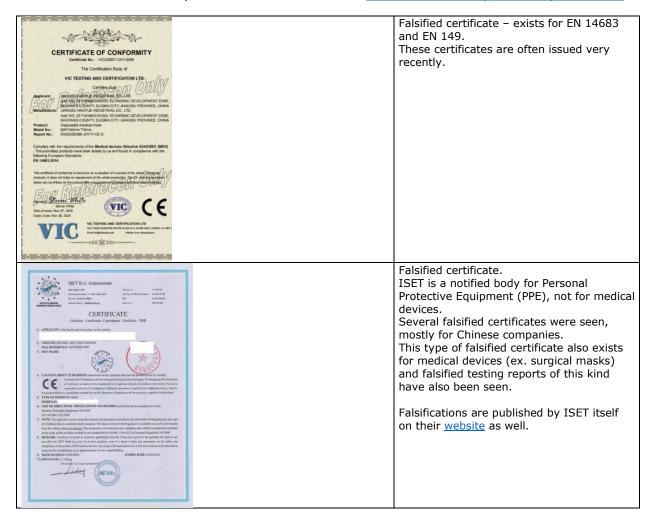

0

Anatalian Prezimite	ICR is not a notified body for medical
Attestation	devices. This kind of attestations is of no value.
of Conformity	This kind of accestations is of no value.
No. ICR Polika/M6 CE	
Now and address "Autor to	
Product states Dipolities Transmission Product systemeted A1.22.33 Toole states	
This Attentions can firms that the product meets the requirements of the following semantive documents and while his his of the documents grain presentation of conferency with manyfall requirements of DeviceS 93/LATEC	
Relevant IC Directive         Medical Device Directive (BUCK)IC           Conforming wassesment procedure         LS Directive (Microsoft Conforming Works Microsoft BUCK)IC	
Causil Control of the 1 of Avera IX of Directive \$342,582 Applied semipline discurrance: 01 14001-300	
Applied Carly Magazimed System 201 Des ACs all emain and all by Classify Magaziment System Certificate means cald. The astronger process take terms all of an acadetare with the program (AC-PA) 00.	
The set of	
Invest date 1.153-2007 Exploritorial date 1.153-2007 The notice displaysies and with the orthocology are regulated by the control Nu ICR Public(200-2041)	
This Antonecies against product having the same ambulant growneeting. Hended use that have been explained and meet the requirements of the Antoneccionid standard.	
AND PE NUMERON AND	
Deeter Rifs Giroseli Wener, 16.0.2020	
ICI Public G. LM. 4. The Thymeres 10, 354 Winesees winesing characteristics of early countering and the third public the public of the publi	
	ICD is not a notified body for Dersonal
SCA)	ICR is not a notified body for Personal
Certificate	Protective Equipment (PPE). The certificate is issued on a 'voluntary
Ne. ICR Polikar/ME202020 CE	basis' and is based on testing results of a
Received and the second and the seco	non-accredited lab.
Name and address of Hours Bo-Technology (Roungblook Holling Co. 185 No.28 Oyum Rock, Handris Form, Handris Form, Compthew S10880.	The certificate does not confirm any
Preduct name: Particular Inspirator XPUS Face Mask Preduct types: \$1965-F13MYZ-21	conformity to EU requirements.
The contracts continue type the proposed meets the independent of the following standards and which has of its handwide give presentation of contraring with executing implements of Regulations 2014(42): Us 16 42(4): 42209	ICR also confirms this on its <u>website</u> .
The cardination process the bare cardinal cardinal and the program (K. 2-47-47). Evaluation takes cardinal double accordance with temports wake by Gaungshoo Benkik Terrafry Services C.a. LLL Salawitory	
Ma, of Inde Anguella. INTERCONSTRUCTION INTERCONSTRUCTURINO INTERCONS	
Equivation date: 1002/205 The mutual adaptions and rights of the certification are regulated by the contract No. KX Heldw2/06/2027	The certificate is of no value.
This certificate applies to produce builty the same attributer (parameters), intended sate, that have been evaluated and meet the requirements of the abovenetioned standards.	
A XE	
Transfer for a fallowed	
Winstein 11. 01. 2000	
d. Ple Popular 8. 6544 Workson www.ispoldk.com, e-with Topoldalification	
ТОО	Conformity certificates /CE certificates
Baustan This first for Technicary Co. Jul.	cannot be issued by Chinese testing
CE Certificate of Conformity	laboratories, only by European notified
CERTIFICATE OF CONFORMITY  CERTIFICATE OF CONFORMED  CERTIFICATE OF CONFOR  CERTIFICATE OF CONFORMED  CERTIFICATE OF CONFORMED  CERTIFICATE OF	bodies.
Angene DERROHAR AND	These certificates have no value.
Aller Constant Section 2015 Biological Section 2015 Bi	
Name         Participant         Paritipant         Participant         P	
The product has some end up that the following opticality ended to ended to a set of the source of t	
Standard DA 19 Addition 20 Addition 20 Addition 20 Additional additational additional additional ad	
EXCE	
Contract Circle Instants Contractions Contract Circle Contractions Contra	
7/7 Date: The could character 201	ECM is a notified body for medical devices,
Image: State	not for Personal Protective Equipment
Helder: Charghine Weijin New Sar Chelling Co. Jul 1 Status Charghine (Co.	(PPE).
Review good: Vulface and	
Pervise good: The presence of	This document only states that the
	manufacturer has drawn up technical
Review output: The interview of a management of the management of	documentation, nothing else.
The accuracy process, the out-shares the time of the second secon	
packing the (Cluss on the pack):     U     Rowlew output     The plane we plane that have a built on the plane of a to support the plane that the plane of a to support the plane that the plane tha	This kind of certificate is not accepted for
	Personal Protective Equipment (PPE) and
A Construction and the large of a formular in th	has little of no value for medical devices; it
Concerting a Structure State S	does not prove any conformity.
Mar Carlos Carlo	The validity of these sections in the
No classical de la contractiva	The validity of these certificates can be
	checked on the <u>website</u> of ECM. The same website page also shows a list of
	fake and falsified ECM certificates.

**FAMHP** 

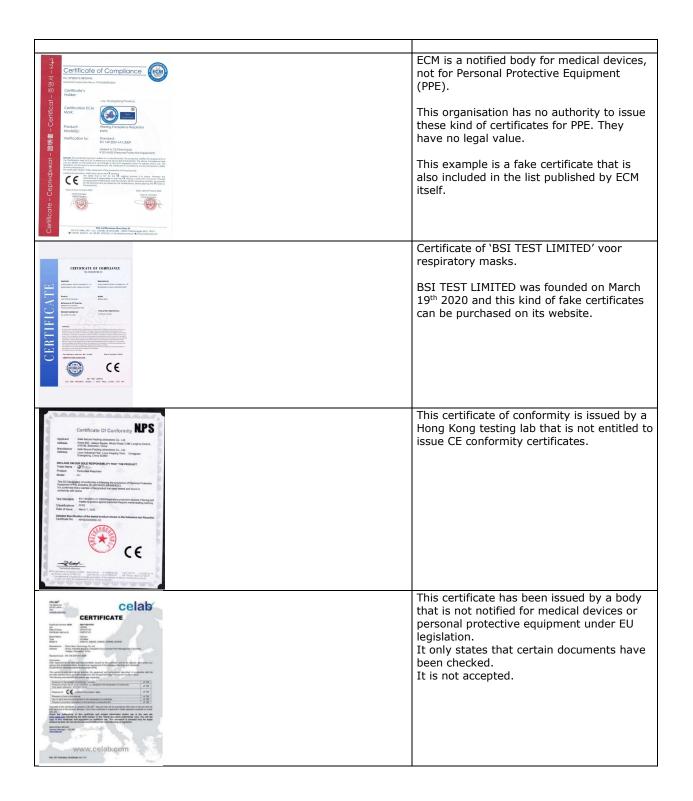

FAMHP

0